

ANALIZA BIAŁEK



Scan for verify



100018380

Laboratory of Analysis

Client: Ultimte Biolabs
Order number: 100018380
Name: ULTIMATE BIOLABS GLOW BLEND
Number of samples: 1 vial

Batch number: -----
Receive date: 2026-09-16
Start date: 2026-09-18
End date: 2026-10-01

Sample identification

Substance	Method of taking a sample	Form
-----	Sample provided by customer	Blue powder in a glass vial

Results

Substance	Sample name	Content	Purity
BPC-157	ULTIMATE BIOLABS GLOW BLEND 70MG	10,68mg	99%
TB-500	ULTIMATE BIOLABS GLOW BLEND 70MG	10,28mg	99%
GHK-Cu	ULTIMATE BIOLABS GLOW BLEND 70MG	54,28mg	99%
BPC-157	ULTIMATE BIOLABS GLOW BLEND 70MG	1419,51m/z	-----
TB-500	ULTIMATE BIOLABS GLOW BLEND 70MG	4963,42m/z	-----
GHK-Cu	ULTIMATE BIOLABS GLOW BLEND 70MG	404,93m/z	-----
Endotoxin Level	ULTIMATE BIOLABS GLOW BLEND 70MG	6,28EU/vial	-----

Research comment

The test sample was applied in the amount of 3µl to the BioBasic 8 Thermo Scientific column. During the course of the analysis with the method a linear gradient in the solutions of H₂O and Acetonitrile with the addition of 0.1% trifluoroacetic acid, peaks of the sought substances appeared. Their contents, when compared to the reference chromatograms, are shown in the table above. Height the measurement error is +-0,05mg. The actual state of the sample sent before the test is presented on the photo below.

Photo of the test sample




Password

SZXZRDEO

Analiza Bialek sp. z o.o.
KRS: 0000966168
NIP: 8992922970
REGON: 521751875

Headquarters and Laboratory:
ul. Duńska 9, 54-427 Wrocław
Budynek DELTA

Lab technician:
Analysis and research specialist
mgr Arkadiusz Zajac



ANALIZA BIAŁEK




Scan for verify




100018380

Chromatogram

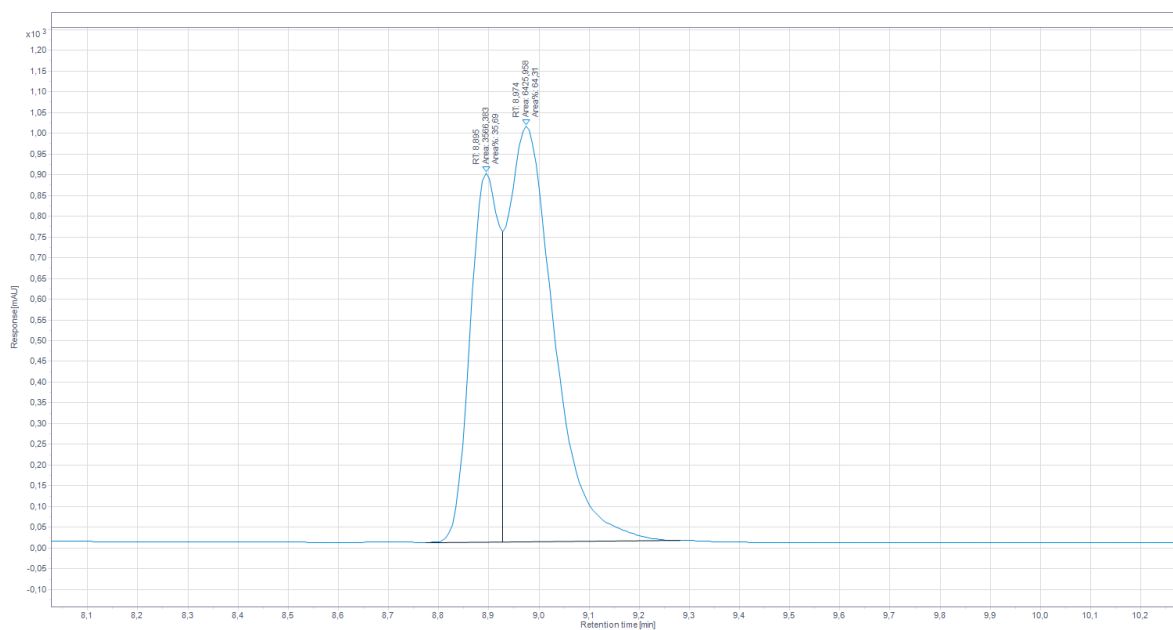

Chromatogram

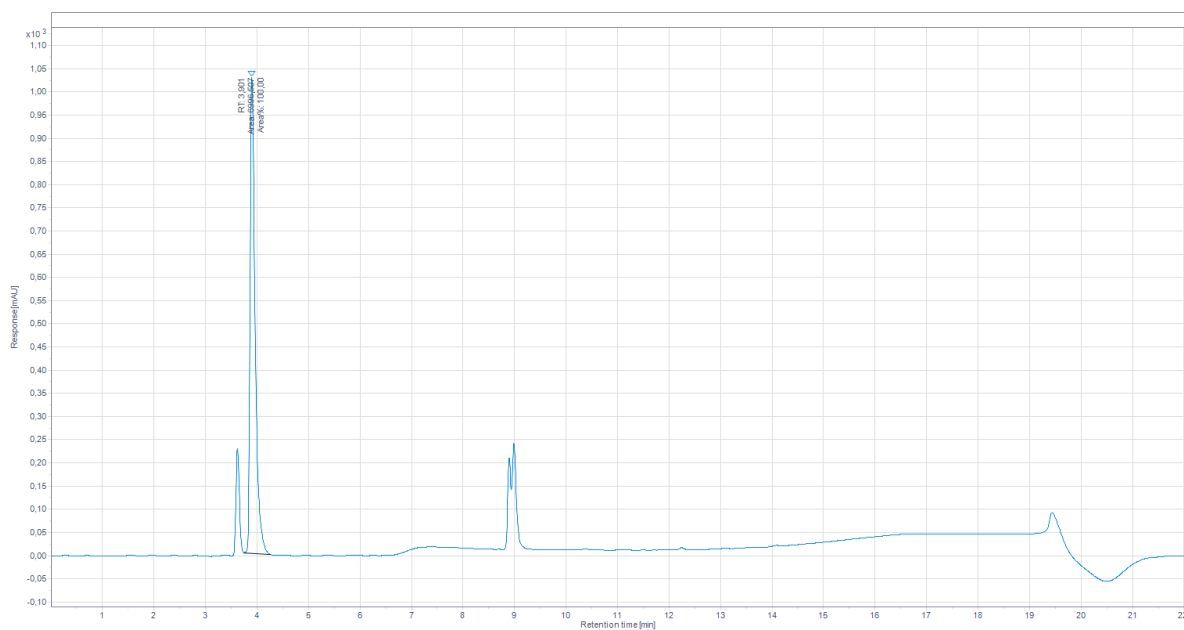

Password

SZXZRDEO

Analiza Białek sp. z o.o.

KRS: 0000966168

NIP: 8992922970

REGON: 521751875

Headquarters and Laboratory:


ul. Duńska 9, 54-427 Wrocław

Budynek DELTA

Lab technician:

Analysis and research specialist

mgr Arkadiusz Zając



ANALIZA BIAŁEK



Scan for verify



100018380

Method

Time	H ₂ O + 0,1% TFA	ACN + 0,1% TFA
0min	95%	5%
2min	95%	5%
12min	5%	95%
15min	5%	95%

Password

SZXZRDEO

Analiza Bialek sp. z o.o.

KRS: 0000966168

NIP: 8992922970

REGON: 521751875

Headquarters and Laboratory:


ul. Duńska 9, 54-427 Wrocław

Budynek DELTA

Lab technician:

Analysis and research specialist

mgr Arkadiusz Zajęc



ANALIZA BIAŁEK



Scan for verify



100018380

Laboratory of Analysis

Client: Ultimte Biolabs
Order number: 100018380
Name: ULTIMATE BIOLABS GLOW BLEND
Number of samples: 1 vial

Batch number: -----
Receive date: 2026-09-16
Start date: 2026-09-18
End date: 2026-10-01

Sample identification

Substance	Method of taking a sample	Form
-----	Sample provided by customer	Blue powder in a glass vial

Results

Test	Sample name	Result
TYMC	ULTIMATE BIOLABS GLOW BLEND 70MG	PASS
TAMC	ULTIMATE BIOLABS GLOW BLEND 70MG	PASS
Presence of presumptive Escherichia Coli	ULTIMATE BIOLABS GLOW BLEND 70MG	NOT DETECTED
Presence of Salmonella Spp.	ULTIMATE BIOLABS GLOW BLEND 70MG	NOT DETECTED

Photo of the test sample



Password

VRRXUWXZ

Analiza Bialek sp. z o.o.
KRS: 0000966168
NIP: 8992922970
REGON: 521751875

Headquarters and Laboratory:
ul. Duńska 9, 54-427 Wrocław
Budynek DELTA

Lab technician:
Analysis and research specialist
mgr Arkadiusz Zajac